



Comparison among the Quantification of Bacterial Pathogens by qPCR, dPCR, and Cultural Methods

Matteo Ricchi^{1*}, Cristina Bertasio², Maria B. Boniotti², Nadia Vicari³, Simone Russo¹, Michela Tilola⁴, Marco A. Bellotti³ and Barbara Bertasi⁴

¹ Istituto Zooprofilattico Sperimentale della Lombardia e dell'Emilia Romagna "Bruno Ubertini," National Reference Centre for Paratuberculosis, Podenzano, Italy, ² Istituto Zooprofilattico Sperimentale della Lombardia e dell'Emilia Romagna "Bruno Ubertini," National Reference Centre for Tuberculosis from *M. bovis*, Brescia, Italy, ³ Istituto Zooprofilattico Sperimentale della Lombardia e dell'Emilia Romagna, National Reference Laboratory for Tularemia, Istituto Zooprofilattico Sperimentale della Lombardia e dell'Emilia Romagna "Bruno Ubertini," Pavia, Italy, ⁴ Istituto Zooprofilattico Sperimentale della Lombardia e dell'Emilia Romagna "Bruno Ubertini," Reparto Tecnologie Acidi Nucleici Applicate Agli Alimenti, Brescia, Italy

OPEN ACCESS

Edited by:

David Rodriguez-Lazaro,
University of Burgos, Spain

Reviewed by:

Learn-Han Lee,
Monash University Malaysia, Malaysia
Ana Elena Dorantes-Acosta,
Universidad Veracruzana, Mexico

*Correspondence:

Matteo Ricchi
matteo.ricchi@izsler.it

Specialty section:

This article was submitted to
Food Microbiology,
a section of the journal
Frontiers in Microbiology

Received: 31 August 2016

Accepted: 08 June 2017

Published: 28 June 2017

Citation:

Ricchi M, Bertasio C, Boniotti MB, Vicari N, Russo S, Tilola M, Bellotti MA and Bertasi B (2017) Comparison among the Quantification of Bacterial Pathogens by qPCR, dPCR, and Cultural Methods. *Front. Microbiol.* 8:1174. doi: 10.3389/fmicb.2017.01174

The demand for rapid methods for the quantification of pathogens is increasing. Among these methods, those based on nucleic acids amplification (quantitative PCRs) are the most widespread worldwide. Together with the qPCR, a new approach named digital PCR (dPCR), has rapidly gained importance. The aim of our study was to compare the results obtained using two different dPCR systems and one qPCR in the quantification of three different bacterial pathogens: *Listeria monocytogenes*, *Francisella tularensis*, and *Mycobacterium avium* subsp. *paratuberculosis*. For this purpose, three pre-existing qPCRs were used, while the same primers and probes, as well as PCR conditions, were transferred to two different dPCR systems: the QX200 (Bio-Rad) and the Quant Studio 3D (Applied Biosystems). The limits of detection and limits of quantification for all pathogens, and all PCR approaches applied, were determined using genomic pure DNAs. The quantification of unknown decimal suspensions of the three bacteria obtained by the three different PCR approaches was compared through the Linear Regression and Bland and Altman analyses. Our results suggest that, both dPCRs are able to quantify the same amount of bacteria, while the comparison among dPCRs and qPCRs, showed both over and under-estimation of the bacteria present in the unknown suspensions. Our results showed qPCR over-estimated the amount of *M. avium* subsp. *paratuberculosis* and *F. tularensis* cells. On the contrary, qPCR, compared to QX200 dPCR, underestimated the amount of *L. monocytogenes* cells. However, the maximum difference among PCRs approaches was $<0.5 \text{ Log}_{10}$, while cultural methods underestimated the number of bacteria by one to two Log_{10} for *Francisella tularensis* and *Mycobacterium avium* subsp. *paratuberculosis*. On the other hand, cultural and PCRs methods quantified the same amount of bacteria for *L. monocytogenes*, suggesting for this last pathogen, PCRs approaches can be considered as a valid alternative to the cultural ones.

Keywords: dPCR, qPCR, bacteria, quantification, pathogens

INTRODUCTION

The advent of molecular tools for the rapid detection of bacterial pathogens has profoundly changed diagnosis methods both in term of rapidity and cost effectiveness (Law et al., 2014). In this regard, an impressive amount of new protocols based on molecular amplification approaches have been developed. These methods are considered alternative or, in some cases, complementary to the classical methods (i.e., cultures).

One of the most popular molecular tools is the polymerase chain reaction (PCR) and, more recently, the quantitative PCR (qPCR), has become one of the most used methodologies for the detection of a wide range of pathogens, including viruses, bacteria, and parasites (Law et al., 2014; Sloots et al., 2015). In addition, this last application also permits the absolute quantification of pathogens present in a given amount of sample. For this purpose, in order to generate calibration curves, standards, containing known amounts of plasmids, genomic DNAs or other nucleic acid molecules (NAs) are run, in parallel with the unknown samples. According to semi-log regression model, it is possible to establish the amount of nucleic acid in unknown specimens (Anonymous, 2012). Based on this feature, and taking into account the efficiency and the dilution steps required for the NA extraction and analysis, it is possible to determine the absolute number of pathogens in the unknown samples (Ricchi et al., 2016).

Another recent PCR-based approach, named digital PCR (dPCR), permits the quantification of the NA present in PCR tubes. Conversely to qPCR, this approach does not require calibration curves for quantification, but it is based on sample partitioning, so that individual nucleic acid molecules are amplified by an end-point PCR and positive partitions can be an estimate of target concentration through Poisson distribution (Hudecova, 2015). Finally, dPCR is considered more robust, reliable and less sensitive to inhibitors than qPCR (Devonshire et al., 2015).

The aim of our study was to compare the quantifications performed by both PCR approaches (qPCR and dPCR) in the enumeration of three pathogen bacteria suspended in unknown water suspensions. The bacteria considered in the study were: *Listeria monocytogenes*, *Francisella tularensis*, and *Mycobacterium avium* subsp. *paratuberculosis* (MAP).

These bacteria grow in solid cultures at different rates, *L. monocytogenes* being the fastest (approximately 1 day), then *F. tularensis* (approximately 3 days) and MAP the slowest (approximately 30–50 days) and since the different growing rates can have an impact in the quantification done by cultural plating (Kralik et al., 2012), the amount of bacteria present in unknown suspensions was quantified by pathogen-specific qPCRs, by two different dPCRs systems, the QX200™ Droplet Digital™ PCR System (Bio-Rad, Berkeley, USA) and the QuantStudio™ 3D digital PCR system (QS3D; Applied Biosystems). The obtained results were also compared with each other and with the relative cultural assays, with the method based on the measure of absorbance at 600 nm and, but only for MAP, direct microbial count (Bürker chamber).

The three bacteria were selected as representative of mycobacteria genus, gram positive, and gram negative bacteria. In more detail, *L. monocytogenes* is a gram positive bacterium responsible for listeriosis, a foodborne illness which predominantly affects pregnant women, elderly people, neonates, and adults with impaired immune systems. Since this pathogen is ubiquitous and it is very difficult to guarantee its absence in many ready to eat products; the European regulation 2073/2005, based on a risk assessment approach, stated the maximum amount that should be present in food, (Anonymous, 2005).

F. tularensis is a gram-negative, facultative intracellular bacteria causing tularaemia, a zoonotic disease that could be fatal to humans and animals. Tularaemia can be transmitted with infected animals or ticks bites, via inhalation or ingestion of contaminated aerosol or food. Due to low infectious dose (as few as 10 microorganisms) and airborne transmission, *Francisella* is currently classified as a category a biological agent (Carvalho et al., 2014).

M. avium subsp. *paratuberculosis* (MAP) is the etiological agent of paratuberculosis (John's Disease), a chronic enteritis affecting wild and domestic ruminants. A possible zoonotic role of MAP in the developing of Crohn' disease is still debated in literature (Chiadini et al., 2012).

Finally, in order to ascertain the possibility of using molecular methods for the quantification of bacterial pathogens, for only *L. monocytogenes*, the level of uncertainty associated to the quantification of each method was evaluated.

MATERIALS AND METHODS

Quantitative PCRs and Digital PCRs qPCRs

The absolute number of bacterial quantity through qPCR was determined using a calibration curve generated with genomic DNA.

The MAP genomic DNA used to build the standards for the absolute quantification of MAP was kindly provided by Dr. Plain from University of Sidney; the *L. monocytogenes* genomic DNA and the *F. tularensis* genomic DNA were extracted from ATCC 13922 and ATCC 6223 strains, respectively. *L. monocytogenes* and *F. tularensis* genomic DNA was initially quantified by QuantiFluor® dsDNA System (Promega, Milan, Italy).

MAP quantification by qPCR targeting the f57 region (f57-qPCR) was performed in 20 μ L (final volume) containing 2x Taqman Universal PCR mastermix (Applied Biosystems), 300 nM primers each and 150 nM Taqman TAMRA Probe (Ricchi et al., 2014, 2016) in a StepOne Plus system (Applied Biosystems). *L. monocytogenes* amplifications were carried out targeting the listeriolysin O (hlyA) gene using primers and probe already described (Traunsek et al., 2011). This last qPCR assay was performed with 2x Taqman Universal PCR mastermix (Applied Biosystems), 600 nM primers each and 200 nM Taqman MGB Probe in CFX96 (Bio-Rad) real-time PCR System. The thermal cycling conditions were: 50°C \times 2 min, 95°C \times 10 min, 45 cycles of 15 s at 95°C, and 1 min at 60°C. *F. tularensis* qPCRs were performed using primers and probe targeting the 23 kDa protein gene, as previously described (Versage et al., 2003). Amplification

was carried out with 2x SsoAdvanced Universal Probes Supermix (Bio-Rad), 600 nM of each primer and 200 nM of Taqman Probe in CFX96 (Bio-Rad) real-time PCR System. The thermal cycling conditions were: 95°C × 2 min, 45 cycles of 5 s at 95°C, and 10 s at 60°C. For each run, at least one negative template control (NTC) was included. C_q determination was performed using the fit point method.

Quantitative PCRs were developed and validated according to the MIQE guidelines (Bustin et al., 2009). This information is available in the Data Sheet 1 (Supplementary Material 1) of the paper.

The qPCR information relative to the performance of the assays was already reported in the original papers or listed in the Data Sheet 1. For each reaction, five points of genomic DNA log-dilution were added in triplicate to each run and used as standards for the absolute bacterial quantification. This was evaluated considering the genome size and the amount of added DNA using a semi-log model based on an excel datasheet (available on request).

dPCRs

Digital PCR reactions were performed in two different systems: QX200™ Droplet Digital™ PCR System (Bio-Rad) and Applied Biosystems® QuantStudio™ 3D digital PCR system (QS3D), for all three bacteria. The reactions were carried out using the same primers and probes concentrations as for qPCRs. Results were expressed as number of bacterial cells per μL.

For Bio-Rad system, five μL of DNA were added to 10 μL of 2X ddPCR™ Supermix for Probes (No dUTP; Bio-Rad), to the specific forward/reverse primers and probe, in a final volume of 20 μL. Droplets were generated using a droplet generator cartridge in a QX200™ Droplet Generator (Bio-Rad), according to the manufacturer's instructions. The droplets emulsion was then loaded into an ABI thermal cycler (Applied Biosystem). Amplification conditions for all three targets were: 10 min at 95°C for enzyme activation, followed by 40 cycles of a two-step thermal profile of 30 s at 94°C (denaturation), 1 min at 60°C (annealing/extension) with a reduced ramp rate of 2°C/s, and a final 10 min vation step at 98°C. Plates were then transferred to a QX200™ Droplet Reader (Bio-Rad). For each run, at least one No Template Control (NTC) was included. All of the thresholds were set up manually to allow the discrimination between positive and negative droplets: two positive droplets were enough to determine a sample as positive, and only the reactions with more than 10,000 accepted droplets were used for analysis. All NTCs resulted negative. In the present study, the number of accepted droplets ranged from 11,439 to 18,415, with a mean of 15,376. Absolute quantification of PCR targets was performed using QuantaSoft™ software version 1.7.4.0917 (Bio-Rad). The mean number of copies per partition (λ), the number of estimated copies per total reaction volume (20 μL), the number of estimated copies per mean effective reaction size were calculated (Pavšič et al., 2016). The mean λ -value was also determined for each sample dilution. The sample concentration expressed as copies per μL was estimated both on the basis of total reaction volume and effective reaction size (Pavšič et al., 2016). On the basis of the droplets volume of 0.85 nL used for

QX200 system, the mean effective reaction size was estimated as 12.99 (± 1.68) μL. Students' tests were used to determine the statistical significance of the sample concentration values, considering the total reaction volume and the effective reaction size.

For the Applied Biosystems QuantStudio™ 3D digital PCR system (QS3D), the reactions were prepared in a final volume of 16 μL, composed by 10.7 μL of Mastermix QuantStudio® 3D Digital PCR (Applied Biosystems, Milan, Italy) and 5.3 μL of DNA at different dilutions; primers and probes were used at the concentrations described for qPCR. Results were expressed as bacterial cells per μL. The reaction mix (15 μL out of 16 μL) was loaded onto the QuantStudio 3D digital PCR chips by using QuantStudio 3D digital PCR chip loader. The amplification conditions for all bacteria were: 96°C × 10 min; 60°C × 2 min, 98°C × 30 s, 39 cycles; 60°C × 2 min. The amplifications were performed in a Proflex™ 2x Flat PCR System. The chips were transferred to a QS3D Instrument for imaging. Data elaboration was executed using the cloud-based QuantStudio 3D Analysis Suite software (version 3.0.03) in the absolute quantification module maintaining automatic settings. For each run, at least one NTC was included. The quality threshold was set at the default value of 0.5, to define the accepted wells and ranged from 10,518 to 18,608 with a mean of 16,838.

Also for QS3D dPCR, the mean number of copies per partition (λ) and the number of estimated copies per total reaction volume (15 μL) for the unknown samples were calculated.

The information relative to the dPCRs, as suggested by MIQE guideline for digital PCR (Huggett et al., 2013), are listed in the Data Sheet 1 (Supplementary Material 1) of the present paper.

Preparation of Unknown Bacterial Suspensions for the Quantification

In order to minimize sources of variability due to different efficiencies of the method chosen during DNA extraction and purification (Devonshire et al., 2015), 5 μl of unknown suspensions were used as templates for qPCRs and dPCRs without any other set up processing (no DNA extraction kits were used). Results were expressed as the number of bacterial cells per μL.

Mycobacterium avium subsp. *paratuberculosis*

A MAP reference strain (ATCC 19698) and two MAP field isolates (IZSLER 623/15 and 22/16) were used. MAP suspensions were prepared according to Logar et al. (2012) and Plain et al. (2014). Briefly, colonies from solid cultures were suspended in distilled water with glass beads (diameter ca. 5 mm) and vortexed for 45 s. The optical density at 600 nM was adjusted to be around 0.7. The suspensions were forced through a syringe (needle 26 G) three times and filtered through a sterile 5 μm filter and then examined in a Bürker chamber to count the number of MAP cells (expressed as MAP cells per mL of suspension). The initial suspensions were 10-fold serially diluted in 1 mL of distilled water in tubes with glass beads (diameter ca. 5 mm) and vortexed for 20 s between dilution steps. One hundred microliters of each dilution were streaked in duplicate onto Petri plates (diameter 9 cm) of Herrold's Egg Yolk Agar with Mycobactin J 2 mg/L

(HEYM) for the determination of MAP concentrations expressed as CFU per μL . Plates were incubated at 37°C and the number of CFU was counted approximately 80 days after the inoculum. For the initial suspensions, the optical density at 600 nm was also recorded three times in BioPhotometer[®] (Eppendorf, Milan, Italy).

The remaining parts of the suspensions (approximately 850 μL) were then submitted to bead beating (Tissue Lyser II, Qiagen, Milan, Italy) for 10 min at 30 Hz in the presence of 300 mg of 150–212 μm -diameter acid-washed glass beads (Sigma Aldrich, Milan, Italy). The suspensions were then heated at 100°C for 20 min, centrifuged at 16,000 g for 5 min and 5 μL of the supernatant were processed by qPCR and dPCRs.

Listeria monocytogenes

Regarding *L. monocytogenes*, three field isolates, IZSLER 133-1/2016, 129516-1/2016, and 424965-2/2016 were used. The strains were prepared as described for MAP isolates and the absorbance read at 600 nm by DU 800 spectrophotometer (Beckman Coulter). Burkler chamber counting was not performed. Plate counting was performed on blood agar as described in ISO 11290-2 (Anonymous, 1998), incubated at 37°C for 24 h. The remaining parts of the suspensions were then heated at 100°C for 20 min and centrifuged at 16,000 g for 5 min. Five microliters were used as the template for qPCR and dPCRs.

Francisella tularensis

A *F. tularensis* reference strain (ATCC 6223) and two field isolates (IZSLER 42055/2008 and 318595/2009) were used. *F. tularensis* suspensions were prepared as previously reported for MAP and *L. monocytogenes*, without glass beads treatment between each dilution. The optical density at 600 nm was recorded but counting through Burkler chamber was not performed. Fifty microliters of each dilution were streaked in duplicate onto Petri plates (diameter 9 cm) on Cysteine Heart Agar (CHA) to determine *F. tularensis* concentrations expressed as CFU per μL . Plates were incubated at 37°C and examined approximately 5 days after the inoculum in order to record the number of CFU.

The remaining parts of the suspensions were then heated at 100°C for 20 min and centrifuged at 16,000 g for 5 min. Five microliters were used as template for qPCR and dPCRs.

Limit of Detection (LOD) and Limit of Quantification (LOQ) of the PCR Assays

The LOD and LOQ for qPCRs and dPCRs were evaluated using genomic DNA for each bacterium. For qPCRs, the limits of detection is represented by 95% of a positive call, herein defined as $\text{LOD}_{95\%}$ were evaluated using genomic DNAs. According to Pavšič (Pavšič et al., 2016), five replicates in two independent runs of serially diluted genomic DNA were analyzed (10 replicates in total), and logit functions instead of the probit functions were used (Burns and Valdivia, 2008). Notably, this approach was also recommended by the OIE Manual of Diagnostic Tests and Vaccines for Terrestrial Animals (Anonymous, 2014). Results were expressed as Log_{10} fg per reaction.

As stated in the above cited paper (Pavšič et al., 2016), the limit of quantification (LOQ) for qPCRs was fixed at the

lowest concentration where all replicates were positive and the coefficient of variation was up to 25%. The same limits were used for LOQ determination for both dPCRs systems (Pavšič et al., 2016), while the LOD for dPCRs was fixed at the lowest concentration where all replicates gave a positive results (Pavšič et al., 2016). Results were expressed as number of cells per μL . The variability of dPCRs was estimated evaluating the intra run and the inter run variations expressed as coefficients of variations. In more detail, intra run variability was evaluated analysing five dilutions tested in five replicates of genomic standard DNAs; the inter run variability was evaluated analysing the same five dilutions in five replicates tested in two independent runs.

Statistical Analysis for the Comparison between PCR Approaches in Unknown Samples

Agreement and linear regression between the different PCR methods were evaluated, after Log_{10} data transformation, according to the statistical approaches proposed by Bland and Altman (Bland and Altman, 1986). Normality of differences between the quantity obtained by the three PCR methodologies for unknown samples was assessed by Shapiro-Wilk test (STATA 12, Texas, USA). Graphs were generated using MATLAB software developed by MathWorks (Massachusetts, USA). The level of uncertainty associated to the quantification for *L. monocytogenes* was evaluated as reported in the ISO/TS 19036 (Anonymous, 2009) for all the methods. In particular, the concentration of *L. monocytogenes* cells (values around the LOQ) were Log_{10} transformed and the expanded uncertainty was calculated with the formula:

$$U = 2 \sqrt{S_R^2 + \frac{0.18861}{\sum c}}$$

where $0.18861/\sum c$ is the variance component due to the Poisson distribution, in which $\sum c$ is the sum of the total numbers of colonies/cells counted. Notably the factor 2 gives a level of confidence of 95%.

S_R is the reproducibility standard deviation calculated with the formula:

$$S_R = \sqrt{\frac{1}{n} \sum_{i=1}^n \frac{(y_{iA} - y_{iB})^2}{2}}$$


where y_{ij} are the Log_{10} transformed data, i is the index of the sample, $i = 10$ to n ($n \geq 10$); j is the index of reproducibility condition, $j = A$ or B .

RESULTS

Determination Of qPCRs and dPCRs Performance

The LOD and LOQ of the three different qPCRs, as well as those of the two dPCR systems, were reported in **Figure 1** and **Table 1**, respectively.

For the f-57 qPCR relative to *M. avium* subsp. *paratuberculosis* (see **Figures 1A,D**), the $\text{LOD}_{95\%}$ was 1.322 Log_{10} fg per reaction (95% CI 0.924–2.739), corresponding to 3.964 genomic

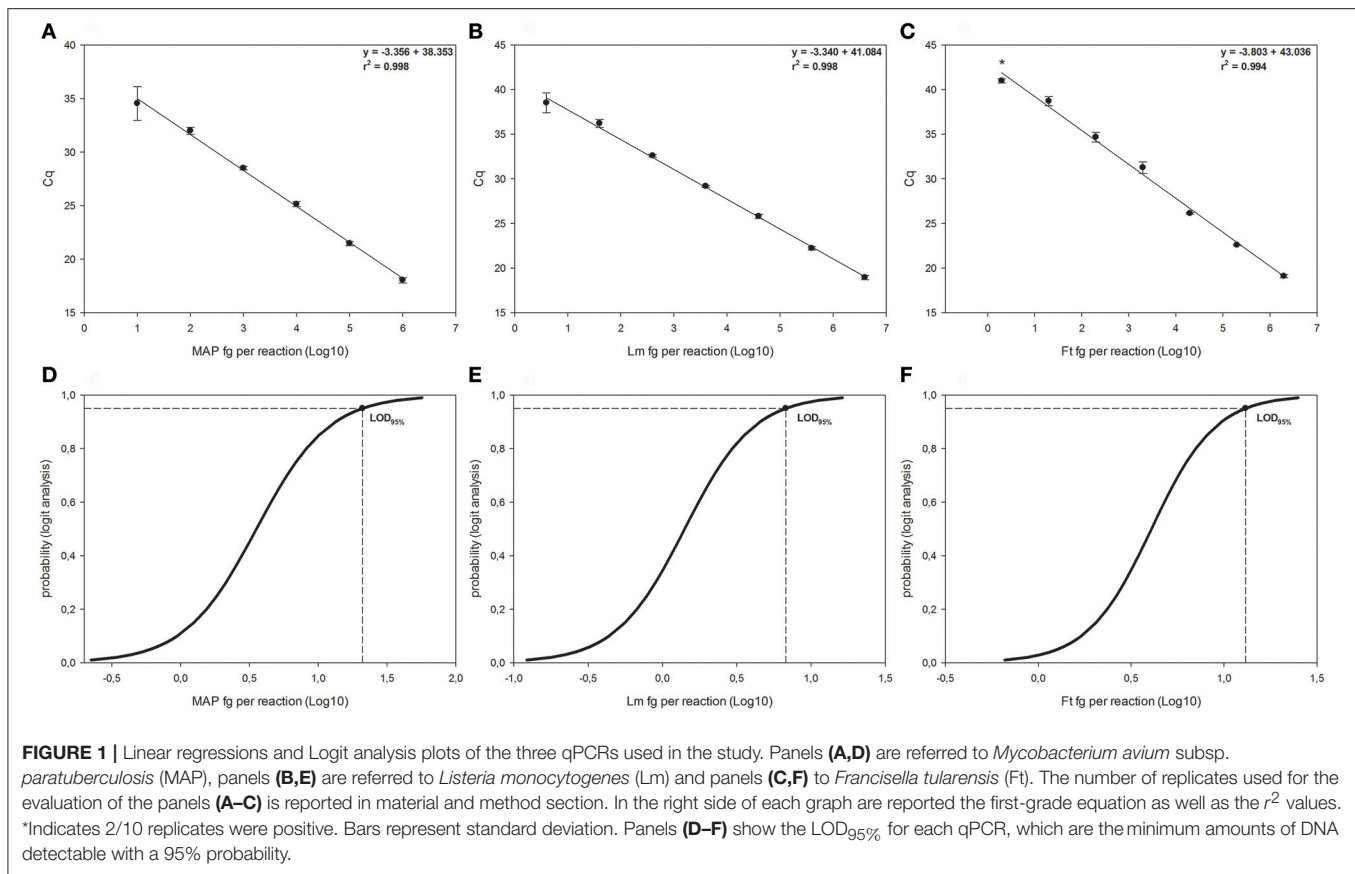

equivalents MAP cells (20.989 fg per reaction divided by 5.295 fg, which is the weight of a single MAP's genome). The LOQ was estimated around 100 fg per reaction, corresponding to 1.889×10^1 genomic equivalent (coefficient of variation 23.419%). The efficiency of the reaction was $98.827 \pm 7.146\%$.

The qPCR for *L. monocytogenes* (see **Figures 1B,E**) showed a $LOD_{95\%}$ of 0.831 Log_{10} fg per reaction (95% CI 0.460–2.104), corresponding to 2.060×10^0 genomic equivalents *L. monocytogenes* cells (6.776 fg per reaction divided by 3.289 fg, which is the weight of a single *L. monocytogenes* genome). The LOQ was fixed at 40 fg per reaction, corresponding to 1.216×10^1 genomic equivalent (coefficient of variation 13.296%), being the concentration below (4 fg per reaction) with a coefficient of variation over 25% (27.265%). The efficiency of the reaction was $98.915 \pm 5.226\%$.

Finally, for *F. tularensis* qPCR (see **Figures 1C,F**), the $LOD_{95\%}$ was 1.116 Log_{10} fg per reaction (95% CI 0.729–3.638), corresponding to 6.382 genomic equivalents *F. tularensis* cells (13.062 fg per reaction divided by 2.047 fg, which is the weight of single *F. tularensis*'s genome). The LOQ was 200 fg per reaction, corresponding to 9.772×10^1 genomic equivalents *F. tularensis* cells (coefficient of variation 4.973%) and the efficiency of the reaction was $80.181 \pm 5.781\%$.

The dynamic range of the reactions varied between one to six Log_{10} fg per reaction for MAP and between approximately one to seven Log_{10} fg per reaction for *L. monocytogenes* and *F. tularensis*.

The performance of the dPCRs are shown in **Table 1**. In order to avoid further variability due to the different setup between different PCR systems and approaches (digital or quantitative), primers and probes were used at the same concentration as for qPCRs. As expected, the dynamic ranges observed were lower than those obtained for the corresponding qPCRs for all bacteria; in fact, for *L. monocytogenes* target DNA over than 10^4 fg per μL , both dPCR systems were saturated and it was not possible to obtain any quantification. The saturation amount was lower for *F. tularensis* (10^3 fg per μL), while it was higher for MAP (10^5 fg per μL).

Contrary to the observations carried out for qPCRs, the QX200 system for MAP and both dPCR systems for *L. monocytogenes* showed LOD and LOQ values overlapped each other, while for the rest of assays, the LOQ values were approximately one Log_{10} higher than LOD (**Table 1**).

The intra run variability (coefficients of variation) obtained from five dilutions, tested in five replicates, ranged from 0.9 to 34.0%, for the QX200 system, and from 3.4 to 64.3% for the QS3D. As expected, we observed an increased variability at the lowest DNA concentrations.

The inter run variability ranged from 1.0 to 25.4% for the QX200 and from 2.1 to 22.6% for the QS3D dPCR. These values were lower than those observed for the intra run, and, in this case, we found this variability increased according to the concentration of tested DNA.

TABLE 1 | Performances of dPCR systems used in the study for detection and quantification of *M. avium* subsp. *paratuberculosis*, *L. monocytogenes*, and *F. tularensis*.

	<i>M. avium</i> subsp. <i>paratuberculosis</i>	<i>L. monocytogenes</i>	<i>F. tularensis</i>
Key Characteristics of dPCR Assay (QX200)			
Dynamic Range (fg per μL) [*]	10^2 – 10^5	10^1 – 10^4	10^0 – 10^3
Dynamic Range (Log_{10} copies/ μL) [°]	1–4	1–4	0–3
LOD— n° of target copies/ μL	$18.120 \pm 2.946^\#$	$10.040 \pm 1.391^\#$	2.204 ± 0.847
LOQ— n° of target copies/ μL	$18.120 \pm 2.946^\#$	$10.040 \pm 1.391^\#$	27.240 ± 3.295
Intra-run Variation: Range of Coefficients of variation (five dilutions tested in five replicates)	± 0.9 to $\pm 15.7\%$	± 3.3 to $\pm 14.1\%$	± 4.4 to $\pm 34.0\%$
Inter-run Variation: Range of coefficient of variation (five dilutions tested five times in two independent replicate runs)	± 6.8 to $\pm 11.9\%$	± 2.0 to $\pm 5.6\%$	± 1.0 to $\pm 25.4\%$
Key Characteristics of dPCR Assay (Quant Studio 3D)			
Dynamic Range (fg per μL) [*]	10^1 – 10^5	10^1 – 10^4	10^0 – 10^3
Dynamic Range (Log_{10} copies/ μL) [°]	0–4	1–4	0–3
LOD— n° of target copies/ μL	2.097 ± 1.345	$13.813 \pm 2.858^\#$	3.367 ± 1.547
LOQ— n° of target copies/ μL	17.769 ± 3.364	$13.813 \pm 2.858^\#$	31.539 ± 4.758
Intra-run Variation: Range of Coefficients of variation (from five dilutions tested in five replicates)	± 3.4 to $\pm 64.3\%$	± 5.9 to $\pm 34.6\%$	± 4.7 to $\pm 39.1\%$
Inter-run Variation: Range of coefficient of variation (five dilutions tested five times in two independent replicate runs)	± 6.7 to $\pm 22.6\%$	± 3.1 to $\pm 8.82\%$	± 2.1 to $\pm 8.4\%$

^{*}These ranges were determined considering the positive signals at LOD level obtained with the same genomic DNA standards used for evaluate the performances of qPCRs.

[°]These ranges were determined considering the LOD.

[#]The value is identical for LOD and LOQ because all replicates were positive and the coefficient of variation is lower than 25%; further details in the material and method section.

Evaluation of the Number of Bacteria in Unknown Suspensions by PCR Approaches

The quantification results obtained for the unknown suspensions at different dilutions, for the three different PCRs (one qPCR and two dPCRs), are shown in **Tables 2–4**. All the NTCs were negative. For the QX200 system, sample concentrations, determined on the basis of total reaction volume and effective reaction size, did not show any statistical difference ($p < 0.05$). Therefore, we decided to use concentration values estimated considering the total reaction volume.

Mycobacterium avium subsp. *paratuberculosis* (MAP)

For MAP, the quantification results showed approximately the same amount of Log_{10} bacterial cells among different PCRs; however, for QS3D dPCR, the system was saturated at the highest concentration and it was not possible to count the number of copies present in the samples for all the analyzed strains. The regression lines and Bland and Altman analyses for MAP (**Figure 2**) were done by taking into account only the dilutions of unknown suspensions which varied from approximately 10^1 MAP cells to 10^3 MAP cells for all the strains tested. The lower limit was chosen because the LOQ for all PCRs was 10^1 MAP cells per μL , while, over 10^3 MAP cells, the QS3D dPCR was saturated. After Log_{10} transformation, the difference between the two dPCRs was not normally distributed ($p = 0.002$) and it was not possible to compare, by Bland and Altman analysis, the

difference between the two dPCR systems. On the contrary, the Log_{10} -difference between qPCR and QS3D dPCR, as well as that between qPCR and the QX200 dPCR, were distributed normally ($p = 0.642$ and $p = 0.523$, respectively). As expected, the linear regressions were well fitted for all comparisons, with r^2 -values between 0.919 and 0.961. Considering the Bland and Altman analysis, the bias for the agreement's range was 0.3 Log_{10} (0.27–0.31 Log_{10}) for both analyses. The zero value fell inside the 95% CI of agreement limits, but p -values vs. zero were 0.006 and 0.003 for difference between qPCR and QS3D and qPCR and QX200, respectively. These results suggested the quantifications by qPCR were slightly higher than those obtained by both dPCR systems.

Listeria monocytogenes

Quantification results of *L. monocytogenes* are shown in **Table 3**. For the highest concentrations of *L. monocytogenes* cells (over 10^4 cells per μL), both dPCR failed to quantify the number of bacteria, while the qPCR quantified up to 10^5 cells per μL . In this case, after Log_{10} transformation, the difference between QS3D dPCR and qPCR was not normally distributed ($p = 0.027$) and it was not possible to make a comparison using Bland and Altman approach for this difference. The Log_{10} -differences QS3D—QX200 and qPCR—QX200 were distributed normally with p -values 0.068 and 0.094, respectively. The interval, analyzed by Bland and Altman, was from 10^1 to 10^3 – 10^4 *L. monocytogenes* cells, according to the LOQs of each PCR approach (see also **Figure 1** and **Table 2**). The linear regressions showed r^2 -values between 0.893 and 0.992, while Bland and Altman analyses (**Figure 3**) exhibited all points falling inside

TABLE 2 | Experimental output of MAP cells obtained by f57-qPCR, f57- QX 200 dPCR and f57- QuantStudio 3D dPCR.

	Dilution	qPCR ^a			dPCR QX 200 ^b				dPCR QuantStudio 3D ^b			
		Mean	SD	Signal ratio ^c	Mean	SD	Mean λ	Signal ratio ^c	Mean	SD	Mean λ	Signal ratio ^c
ATCC 19698	-1	3.62×10^4	1.33×10^4	12/12	1.3×10^4	7.92×10^2	2.76	2/4	Saturated	Saturated		/
	-2	2.60×10^3	1.06×10^3	12/12	1.54×10^3	7.82×10^1	0.32	4/4	5.00×10^2	3.46×10^1	0.38	2/2
	-3	2.68×10^2	1.43×10^2	12/12	1.70×10^2	1.31×10^1	0.04	4/4	1.49×10^2	3.12×10^1	0.04	2/2
	-4	3.66×10^1	2.19×10^1	12/12	1.31×10^1	2.66×10^0	0.00	4/4	1.22×10^1		0.02	1/2
	-5	6.41×10^0	4.78×10^0	8/12	2.16×10^0	5.91×10^{-1}	0.00	4/4	2.01×10^0	8.77×10^{-1}	0.00	2/2
	-6	0	0		1.09×10^0	4.03×10^{-1}	0.00	4/4	1.72×10^0	0.95×10^{-1}	0.00	2/2
	-7	0	0		6.10×10^{-1}	7.57×10^{-1}	0.00	2/4	4.89×10^{-1}	0.30×10^{-1}	0.00	2/2
IZSLER 623/15	-1	4.98×10^4	1.37×10^4	12/12	2.21×10^4	1.14×10^4	5.74	4/4	Saturated	Saturated		/
	-2	4.29×10^3	1.20×10^3	12/12	2.00×10^3	2.09×10^2	0.44	4/4	2.25×10^3	1.88×10^2	0.57	2/2
	-3	5.09×10^2	1.41×10^2	12/12	1.85×10^2	1.37×10^1	0.04	4/4	1.83×10^2	3.05×10^1	0.05	2/2
	-4	5.46×10^1	1.75×10^1	12/12	1.48×10^1	1.46×10^0	0.00	4/4	1.72×10^1	7.47×10^0	0.00	2/2
	-5	7.02×10^0	3.38×10^0	12/12	2.47×10^0	4.82×10^{-1}	0.00	4/4	1.43×10^0	1.03×10^0	0.00	2/2
	-6	2.44×10^0	1.83×10^0	10/12	4.93×10^{-1}	3.03×10^{-1}	0.00	3/4	2.50×10^0	2.78×10^0	0.00	1/2
	-7	8.03×10^{-1}	6.64×10^{-1}	3/12	2.70×10^{-1}	3.77×10^{-1}	0.00	1/4	5.23×10^{-1}	4.29×10^{-1}	0.00	2/2
IZSLER 22/16	-1	2.17×10^4	8.31×10^3	12/12	1.62×10^4	3.67×10^3	2.77	4/4	Saturated	Saturated		2/2
	-2	1.26×10^3	2.55×10^2	12/12	1.12×10^3	4.59×10^1	0.24	4/4	1.35×10^3	4.27×10^1	0.34	2/2
	-3	1.03×10^2	1.99×10^1	12/12	8.36×10^1	5.36×10^0	0.02	4/4	1.06×10^2	3.96×10^{-1}	0.03	2/2
	-4	1.21×10^1	4.82×10^0	12/12	1.10×10^1	2.23×10^0	0.00	4/4	9.47×10^0	1.09×10^0	0.00	2/2
	-5	1.57×10^0	1.02×10^0	12/12	1.93×10^0	7.48×10^{-1}	0.00	4/4	1.53×10^0	2.14×10^{-1}	0.00	2/2
	-6	8.55×10^{-1}	6.50×10^{-1}	10/12	3.50×10^{-1}	2.95×10^{-1}	0.00	3/4	4.80×10^{-1}	3.42×10^{-1}	0.00	2/2
	-7	3.07×10^{-1}	7.25×10^{-2}	4/12	4.20×10^{-1}	1.48×10^{-1}	0.00	4/4	6.26×10^{-1}	5.20×10^{-1}	0.00	2/2

^aNumber of MAP cells/ μ L in the pure cultures/suspensions evaluated by f57-qPCR. Data are shown as mean and standard deviation of four qPCR runs in triplicated.

^bNumber of MAP cells/ μ L in the pure cultures/suspensions evaluated by f57-dPCRs. Data are shown as mean and standard deviation of two dPCR runs in duplicated for QX200, and one dPCR run in duplicated for QuantStudio 3D.

^cNumber of positive or acceptable replicates/total number of replicates.

the interval covered by the 95% CI (Figure 3B). The bias of agreement was approximately zero for the comparison between dPCRs ($p = 0.160$), while the comparison between qPCR and QX200 dPCR, showed a bias of -0.44 Log_{10} ($p < 0.001$). This result underlined how the qPCR quantification underestimated the number of *L. monocytogenes* cells in comparison to dPCRs. Notably, the intervals defined by the 95% CI for *L. monocytogenes* were narrower than those for MAP, and the zero value never fell within the intervals.

Francisella tularensis

The results obtained for *F. tularensis* are shown in Table 4 and Figure 4. Also in this case, at the highest concentrations of bacterium, both dPCR systems were saturated and it was not possible to quantify the number of cells present in the unknown suspensions (Table 4). For this reason, and according to the results shown in Table 1 and Figure 1 about the LOQ, the dilutions of unknown suspensions taken into account for the Bland and Altman analysis (Figure 4) were from 10^1 to 10^3 . The Log_{10} -differences among the three PCR approaches were distributed normally, with p -values of 0.505, 0.994 and 0.935 for QS3D—QX200, qPCR—QS3D and qPCR —QX200, respectively. The linear regressions showed r^2 -values between

0.782 and 0.927. Bland and Altman analysis (Figure 4) showed a bias for the agreement's range from -0.14 to 0.3 Log_{10} for all the comparisons, with the zero value falling within 95% CI of the agreement's limits. Overall, all PCR approaches quantified the same amount of bacteria, with the exception of the difference between qPCR—QX200 dPCR in which the p -value of the bias was 0.048. However, it should be noted that the limits of agreement are indeed wider than those previously obtained for MAP and *L. monocytogenes*, underlining a certain degree of variability in the quantification of *F. tularensis*.

Evaluation of the Number of Bacteria in Unknown Suspensions by Other Methods

The results regarding the quantification obtained with “non-molecular methods” are shown in Table 5. For MAP, the direct counting by Burker chamber underestimated the number of bacterial cells for approximately one Log_{10} than the quantification done by PCR approaches, this difference rose up to two Log_{10} for plate counting method. *F. tularensis* showed similar results for plate counting, while for *L. monocytogenes* there were no differences. This last result allowed the assessment of the reproducibility for the quantification of *L. monocytogenes* obtained by both PCR approaches and cultural assay.

TABLE 3 | Experimental output of *L. monocytogenes* cells obtained by hlyA-qPCR, hlyA-QX200 dPCR and hlyA-QuantStudio 3D dPCR.

	Dilution	qPCR ^a			dPCR QX200 ^b				dPCR QuantStudio 3D ^b			
		Mean	SD	Signal ratio ^c	Mean	SD	Mean λ	Signal ratio ^c	Mean	SD	Mean λ	Signal ratio ^c
IZSLER 133/1/16	No dil	4.93×10^6	1.35×10^6	4/4	NT				NT			
	-1	5.33×10^5	8.78×10^4	4/4	NT				NT			
	-2	5.94×10^4	1.55×10^3	4/4	Saturated	Saturated	Saturated	2/2	Saturated	Saturated		2/2
	-3	4.86×10^3	7.37×10^2	4/4	1.72×10^4	1.41×10^2	3.65	2/2	1.95×10^4	/		1/2
	-4	3.40×10^2	4.80×10^1	4/4	1.24×10^3	5.94×10^1	0.26	2/2	1.53×10^3	1.15×10^2	0.38	2/2
	-5	2.89×10^1	2.07×10^0	4/4	1.30×10^2	1.98×10^0	0.03	2/2	1.90×10^2	2.53×10^0	0.05	2/2
	-6	2.75×10^0	9.59×10^{-2}	4/4	1.26×10^1	8.50×10^{-1}	0.00	2/2	1.79×10^1	5.70×10^{-1}	0.00	2/2
IZSLER 129516/1/16	No dil	3.00×10^6	1.26×10^5	4/4	NT				NT			
	-1	2.31×10^5	1.05×10^4	4/4	NT				NT			
	-2	2.32×10^4	2.98×10^3	4/4	Saturated	Saturated	Saturated	2/2	Saturated	Saturated		2/2
	-3	1.65×10^3	4.38×10^2	4/4	5.53×10^3	1.16×10^3	1.17	2/2	6.63×10^3	4.14×10^2	1.67	2/2
	-4	1.58×10^2	5.32×10^1	4/4	6.94×10^2	8.49×10^0	0.15	2/2	7.48×10^2	9.18×10^1	0.19	2/2
	-5	1.11×10^1	4.38×10^0	4/4	5.84×10^1	4.53×10^0	0.01	2/2	6.58×10^1	2.49×10^0	0.02	2/2
	-6	1.07×10^0	6.60×10^{-1}	4/4	5.84×10^0	1.92×10^0	0.00	2/2	7.86×10^0	6.90×10^{-2}	0.00	2/2
IZSLER 424965/2/16	No dil	1.91×10^6	3.19×10^5	4/4	NT				NT			
	-1	2.18×10^5	3.98×10^4	4/4	NT				NT			
	-2	2.92×10^4	3.55×10^3	4/4	Saturated	Saturated	Saturated	2/2	Saturated	Saturated		2/2
	-3	2.16×10^3	1.66×10^2	4/4	8.20×10^3	1.78×10^2	1.74	2/2	5.82×10^3	5.59×10^3	1.46	2/2
	-4	1.52×10^2	1.33×10^1	4/4	7.14×10^2	1.41×10^1	0.15	2/2	7.43×10^2	1.67×10^2	0.19	2/2
	-5	1.45×10^1	1.39×10^{-1}	4/4	8.02×10^1	5.37	0.02	2/2	9.0×10^1	1.05×10^1	0.02	2/2
	-6	1.2×10^0	2.61×10^{-1}	4/4	6.40×10^0	0	0.00	2/2	1.3×10^1	9.10×10^{-1}	0.00	2/2
	-7	6.45×10^{-2}	1.21×10^{-2}	4/4	1.04×10^0	6.80×10^{-1}	0.00	2/2	1.44×10^0	2.00×10^{-1}	0.00	2/2

NT, not tested.

^aNumber of *L. monocytogenes* cells/ μ L in the pure cultures/suspensions evaluated by hlyA-qPCR. Data are shown as mean and standard deviation of two qPCR runs in duplicated.

^bNumber of *L. monocytogenes* cells/ μ L in the pure cultures/suspensions evaluated by hlyA-dPCRs. Data are shown as mean and standard deviation of one dPCR runs in duplicated for both dPCR platforms.

^cNumber of positive or acceptable replicates/total number of replicates.

Evaluation of the Level of Uncertainty for *L. monocytogenes* Associated with the Methods

The levels of uncertainty for *L. monocytogenes* for each method is shown in Table 6. The uncertainty associated with PCR methods was similar or lower to that associated with the cultural assay.

DISCUSSION

The aim of our work was to evaluate if the quantifications obtained by qPCR were comparable to those obtained by two different dPCR systems. Additionally, a comparison among PCR approaches and non-molecular methods was also evaluated.

All the bacteria analyzed in the study are human or animal pathogens and their detection, and quantification, for diagnostic purposes, is relevant, such as during the development of risk exposure analysis models. In these models, the quantification of the real amount of bacteria in a given sample plays a crucial role in the definition of risk (Halder et al., 2010). Therefore, the

interest in developing faster and reliable quantitative methods for detection and quantification is becoming a very important issue in microbiology. This is particularly relevant for some pathogens characterized by slow cultural growth rates (e.g., MAP), but generally, rapidity can be advantageous for detection and quantification of all pathogens. In this regard, some risk models have already been proposed for MAP (Nauta and van der Giessen, 1998; Boulais et al., 2011), *F. tularensis* (Wood et al., 2014) and *L. monocytogenes* (Halder et al., 2010).

According to the Minimum Information for Publication of Quantitative Real-Time PCR experiments (Bustin et al., 2009) and the Minimum Information for Publication of Quantitative Digital PCR Experiments (Huggett et al., 2013) guidelines we provided here data about the performances of the qPCRs and dPCRs used in the study and aimed at quantifying of MAP, *L. monocytogenes* and *F. tularensis*. In order to assess if primers and probes can work in the same way for both qPCR and dPCR, the LOD, LOQ, and the other performance parameters of all dPCRs were done without any further specific reaction optimization and compared to those observed for qPCRs.

TABLE 4 | Experimental output of *F. tularensis* cells obtained by 23 kDa gene -qPCR, 23 kDa gene QX200-dPCR and 23 kDa gene-QuantStudio 3D dPCR.

	Dilution	qPCR ^a			dPCR QX200 ^b				dPCR QuantStudio 3D ^b			
		Mean	SD	Signal ratio ^c	Mean	SD	λ	Signal ratio ^c	Mean	SD	λ	Signal ratio ^c
ATCC 6223	No dil	8.26×10^5	1.27×10^5	9/9	NT				NT			
	-1	1.10×10^5	1.58×10^4	9/9	Saturated	Saturated	Saturated		Saturated			
	-2	8.89×10^3	2.45×10^3	9/9	1.10×10^3	1.99×10^2	0.23	4/4	6.49×10^3	1.82×10^3	1.63	2/2
	-3	7.11×10^2	2.62×10^2	9/9	5.44×10^2	1.37×10^2	0.12	4/4	1.06×10^3	1.24×10^1	0.27	2/2
	-4	5.38×10^1	2.30×10^1	9/9	1.09×10^2	1.46×10^1	0.02	4/4	1.15×10^2	6.46×10^0	0.03	2/2
	-5	2.58×10^0	1.56×10^0	9/9	1.09×10^1	4.12×10^0	0.00	4/4	1.18×10^1	/		1/2
	-6	2.10×10^{-1}	8.64×10^{-2}	9/9	2.19×10^0	6.98×10^{-1}	0.00	4/4	3.89×10^0	/		1/2
IZSLER 42055/1/08	No dil	4.06×10^6	1.51×10^6	9/9	NT				NT			
	-1	5.09×10^5	1.40×10^5	9/9	Saturated	Saturated	Saturated		Saturated			
	-2	2.90×10^4	7.00×10^3	9/9	1.01×10^4	5.15×10^3	2.14	4/4	6.46×10^3	1.66×10^2	1.63	2/2
	-3	2.77×10^3	1.27×10^3	9/9	6.36×10^2	4.89×10^2	0.14	4/4	3.43×10^2	2.85×10^1	0.06	2/2
	-4	3.04×10^2	3.84×10^1	9/9	2.04×10^2	1.21×10^2	0.04	4/4	1.11×10^2	5.66×10^0	0.03	2/2
	-5	1.26×10^1	5.10×10^0	9/9	3.12×10^1	1.16×10^1	0.01	4/4	3.00×10^1	2.67×10^0	0.01	2/2
	-6	1.67×10^0	1.08×10^0	9/9	2.16×10^0	6.75×10^{-1}	0.00	4/4	2.11×10^0	8.77×10^{-1}	0.00	2/2
IZSLER 31895/1/09	No dil	5.77×10^6	9.32×10^5	9/9	NT				NT			
	-1	5.08×10^5	3.54×10^4	9/9	Saturated	Saturated	Saturated		Saturated			
	-2	1.30×10^4	3.08×10^3	9/9	6.70×10^3	1.22×10^2	1.42	2/2	7.13×10^3	5.10×10^2	1.79	2/2
	-3	1.07×10^3	2.58×10^2	9/9	1.44×10^3	8.32×10^2	0.31	2/2	8.39×10^2	7.28×10^{-1}	0.21	2/2
	-4	3.31×10^1	8.17×10^0	9/9	7.68×10^1	1.13×10^0	0.02	2/2	1.30×10^2	3.42×10^0	0.03	2/2
	-5	9.33×10^{-1}	4.47×10^{-1}	9/9	6.74×10^0	4.04×10^0	0.00	2/2	1.12×10^1	1.94×10^0	0.00	2/2
	-6	6.25×10^{-2}	4.00×10^{-2}	9/9	9.20×10^{-1}	9.05×10^{-1}	0.00	2/2	1.14×10^0	1.27×10^0	0.00	2/2

NT, not tested.

^aNumber of *F. tularensis* cells/ μ L in the pure cultures/suspensions evaluated by 23 kDa gene-qPCR. Data are shown as mean and standard deviation of three qPCR runs in triplicate.

^bNumber of *F. tularensis* cells/ μ L in the pure cultures/suspensions evaluated by 23 kDa gene -dPCRs. Data are shown as mean and standard deviation of two dPCR runs in duplicated for QX200 dPCR and one dPCR run in duplicate for QuantStudio 3D dPCR (with the exception of strain IZSLER 31895/1/09 in which also QX200 dPCR was run only once in duplicate).

^cNumber of positive or acceptable replicates/total number of replicates.

Comparison between qPCR and dPCR quantification was performed on a panel of bacterial suspension samples. During the estimation of the titres in the unknown samples, Bland and Altman approach was carried out considering only a few of the tested samples. In fact, it was not possible to include more points in these analyses because: (i) for qPCRs, the limits of quantification (coefficient of variation <25%) did not permit the inclusion of the lowest concentrations, (ii) the dPCR systems were saturated at the highest concentrations. So the available range to perform the analyses was restricted from one to three-four Log₁₀ cells per μ L.

Despite the aforementioned limits, the linear regressions and the Bland and Altman analyses (these last when the differences in Log₁₀ transformed data were normally distributed) for both dPCR platforms, showed a strong correlation (r^2 -values 0.961, 0.992, and 0.782 for MAP, *L. monocytogenes* and *F. tularensis*, respectively). Moreover, both systems quantified a very similar amount of bacteria. However, the analysis of the differences in quantification among qPCR and dPCRs showed that f57-qPCR over estimated, by a 0.3 Log₁₀, the number of MAP cells respect to both the dPCR platforms (p -values 0.06 and 0.03; **Figures 2C,E**). The overestimation effect on the quantification

of microorganisms by qPCR was also recently observed for in the quantification of *M. tuberculosis* (Devonshire et al., 2016) and others works addressed to the quantification of virus (Boizeau et al., 2014; Gosselin-Theberge et al., 2016; Supplementary Material 2). Similarly, also 23 kDa gene-qPCR for the quantification of *F. tularensis* over estimated by 0.3 Log₁₀ the number of cells (p -value 0.048), (**Figure 4E**), but only considering the difference between qPCR and QX200, while between qPCR and QS3D no difference was observed (0.16 Log₁₀ but $p = 0.35$).

On the other hand, other papers reported a general agreement in the amount of target NAs quantified by qPCR and dPCR, both for virus (Hayden et al., 2013; Pavšič et al., 2016) as well as for bacterial quantifications (Verhaegen et al., 2016; Wang et al., 2016; Witte et al., 2016).

Finally, the comparison between the QX200 platform and qPCR for *L. monocytogenes*, showed qPCR can underestimate the number of cells by 0.44 Log₁₀ ($p < 0.001$) and, according to the linear regression curve (**Figure 3C**), also the comparison between qPCR and QS3D dPCR showed an underestimation of the cells number by qPCR. In this regard, two recent papers reported similar results: one was addressed to the quantification

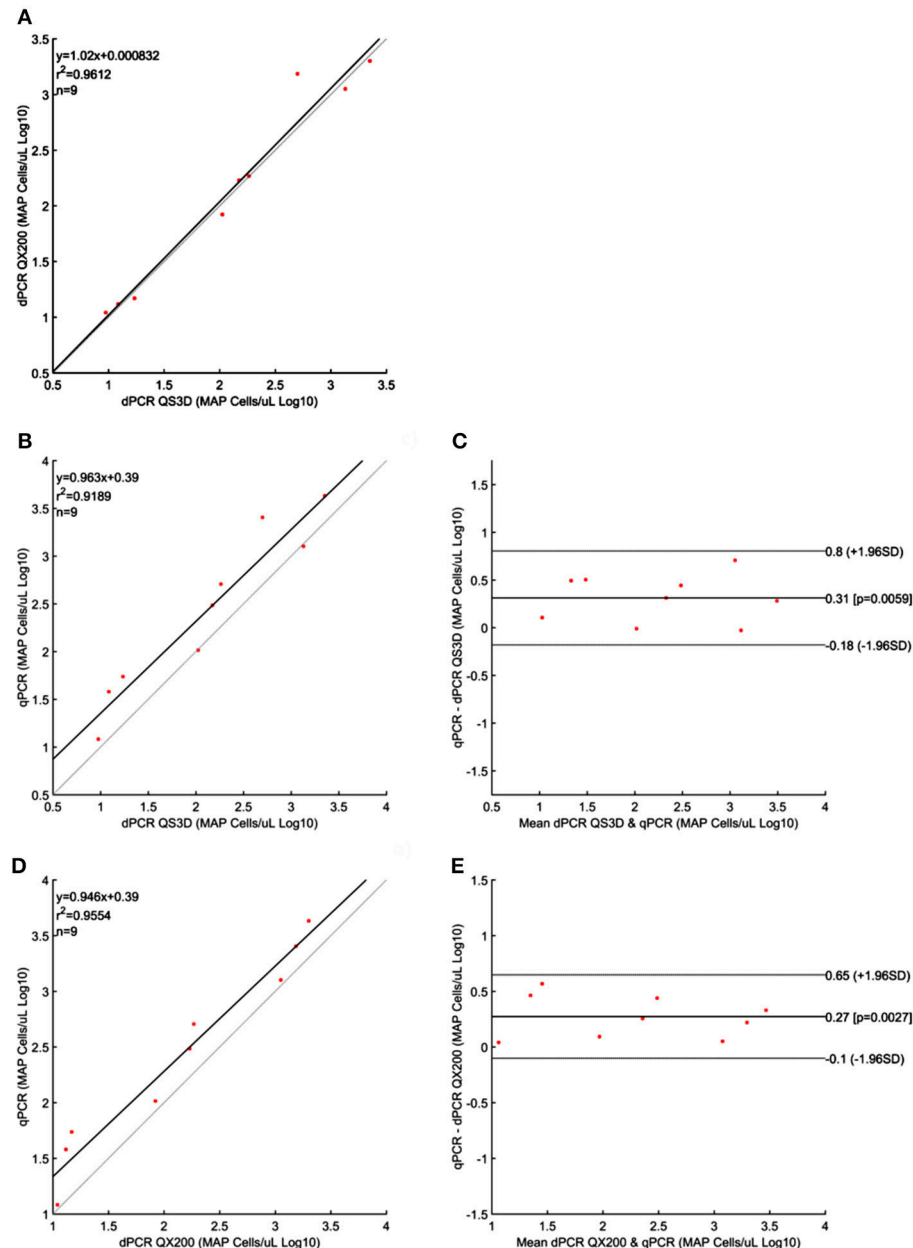


FIGURE 2 | Linear regressions and Bland and Altman analyses of *Mycobacterium avium* subsp. *paratuberculosis* (MAP) cells in unknown samples obtained by dPCRs (QuantStudio 3D and QX200) and qPCR. **(A)** Linear regression between the two dPCRs; **(B)** Linear regression of dPCR QuantStudio 3D and qPCR; **(C)** Bland and Altman analysis of dPCR QuantStudio 3D and qPCR; **(D)** Linear regression of dPCR QX200 and qPCR; **(E)** Bland and Altman analysis of dPCR QX200 and qPCR. Bland and Altman analysis between the two dPCRs platform was not possible because the differences were not normally distributed. Data were reported as Log_{10} cells per μL . The gray lines in linear regression plots represent the ideal regression value.

poultry pathogens (Rothrock et al., 2013) and the other to the quantification of *Campylobacter jejuni* (Papic et al., 2017). A table summarizing these observations is reported in Data Sheet 2 (Supplementary Material 2).

Digital PCR generally is accredited to provide more accurate measurements than qPCR, because it is less affected by the presence of inhibitors and by poor amplification efficiency

than qPCR (Hoshino and Inagaki, 2012; Hudecova, 2015; Pavšič et al., 2015); moreover it is not affected at all by the requirement of NA standards. In fact, it gives an absolute estimate of concentration, through the partition of the sample in template individual reactions. Therefore, dPCR does not need any standards for the generation of calibration curves.

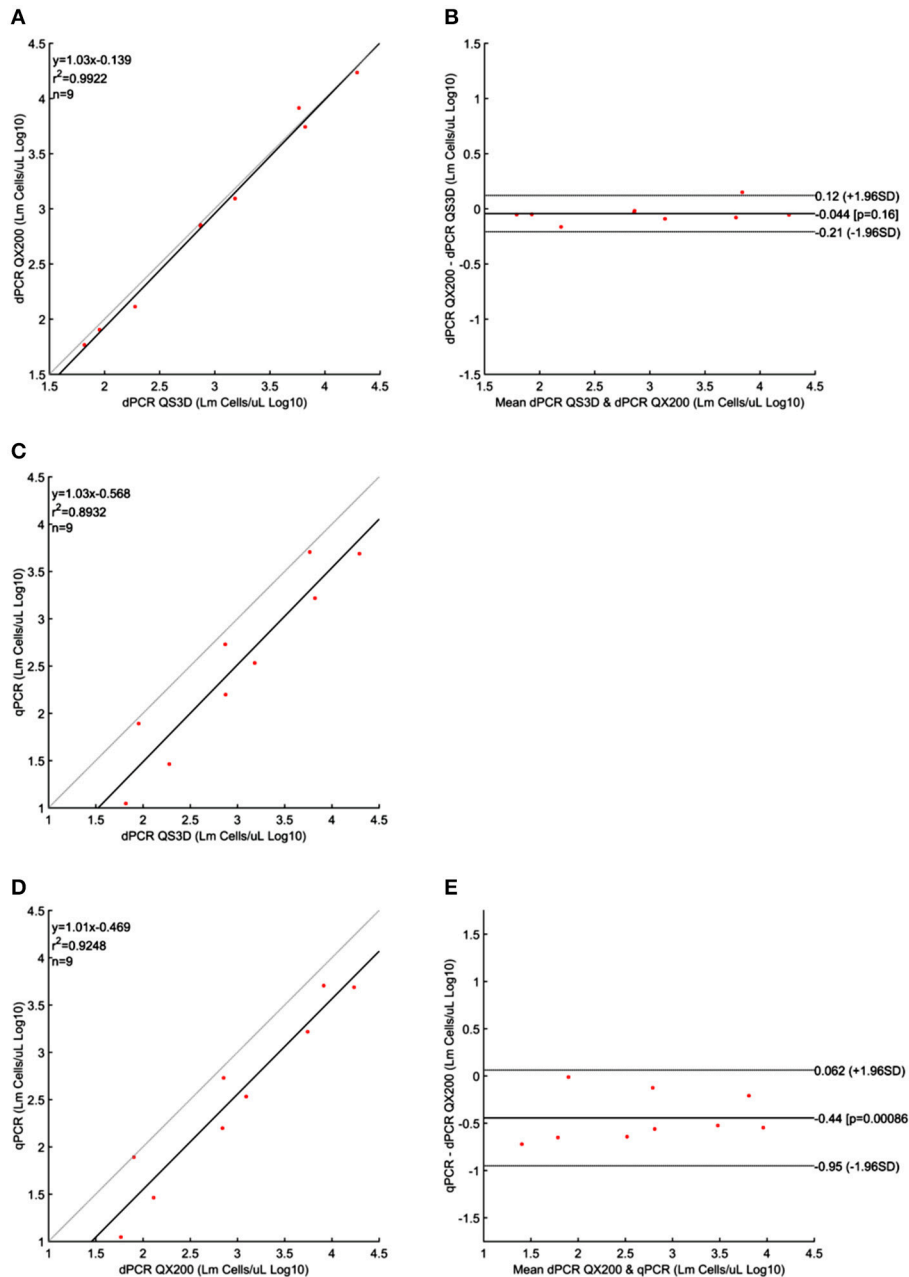


FIGURE 3 | Linear regressions and Bland and Altman analyses of *L. monocytogenes* (Lm) cells in unknown samples obtained by dPCRs (QuantStudio 3D and QX200) and qPCR. **(A)** Linear regression between the two dPCRs; **(B)** Bland and Altman analysis between the two dPCRs; **(C)** Linear regression of dPCR QuantStudio 3D and qPCR; **(D)** Linear regression of dPCR QX200 and qPCR; **(E)** Bland and Altman analysis of dPCR QX200 and qPCR. Bland and Altman analysis between QuantStudio 3D and qPCR was not possible because the differences were not normally distributed. Data were reported as Log_{10} cells per μL . The gray lines in linear regression plots represent the ideal regression value.

Despite its independence on standard curves, compared to qPCR, dPCR is more time consuming and labor intensive. Nevertheless, excluding the initial fee for acquiring the system and considering a run section of 50 samples, the cost of the analysis was less for dPCR (QX200; 3.16 € per sample) than for qPCR (10.80 € per sample).

Some limitations are also present in dPCR systems. In our study, as above mentioned, when pure genomic standards DNA were used at the highest concentration, both dPCR systems were saturated and it was not possible to quantify the number of bacteria. The dynamic range of dPCRs was limited by the number of available partitions, which were around 20,000 for both QX200 and QSD3, while the qPCRs showed higher dynamic ranges.

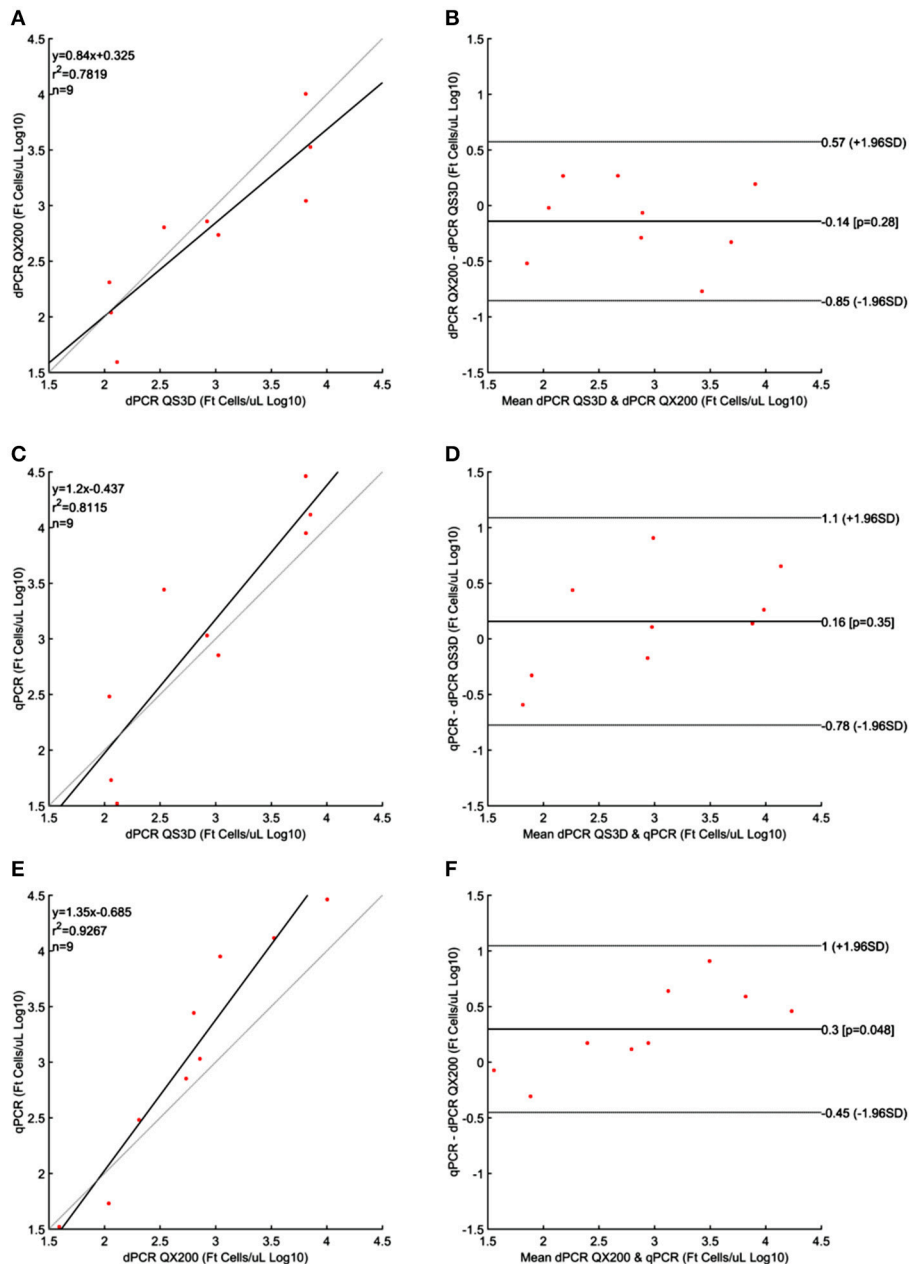


FIGURE 4 | Linear regressions and Bland and Altman analyses of *F. tularensis* (Ft) cells in unknown samples obtained by dPCRs (QuantStudio 3D and QX200) and qPCR. **(A)** Linear regression between the two dPCRs; **(B)** Bland and Altman analysis between the two dPCRs; **(C)** Linear regression of dPCR QuantStudio 3D and qPCR; **(D)** Bland and Altman analysis of dPCR QuantStudio 3D and qPCR; **(E)** Linear regression of dPCR QX200 and qPCR; **(F)** Bland and Altman analysis of dPCR QX200 and qPCR. Data were reported as Log_{10} cells per μL . The gray lines in linear regression plots represent the ideal regression value.

The comparison between quantification by PCR approaches and cultural methods showed some differences, which appear associated to the specific time of growth for each microorganism. In particular, MAP required a very long time to grow (at least 4 weeks) and our results confirmed previous observations in which there is a difference from one to two Log_{10} between plate counting method and PCRs (Herthnek et al., 2008; Kralik et al., 2012; Table 5). Instead, the difference between PCRs and direct

counting method was about one Log_{10} . This could be particularly relevant, because some papers used the direct count method to determine the number of MAP cells during the assessment of LOD for PCR assays (Tasara and Stephan, 2005; Plain et al., 2014).

Comparison between plate counting and PCRs for *F. tularensis*, which has a time of growth in culture of 4–5 days, showed results similar to those obtained for MAP, but the difference between the two methods was less evident. In order to

TABLE 5 | Quantification of the unknown water suspensions carried out by PCR approaches and non-molecular methods.

Strain	<i>Mycobacterium avium</i> subsp <i>paratuberculosis</i>			<i>Listeria monocytogenes</i>			<i>Francisella tularensis</i>		
	ATCC 19698	IZSLER 623/15	IZSLER 22/16	IZSLER 133/1/16	IZSLER 129516/1/16	IZSLER 424965/2/16	ATCC 6223	IZSLER 42055/08	IZSLER 318595/09
Direct count ^a	3.7×10^4	3.6×10^4	3.5×10^4						
Absorbance ^b	0.06	0.09	0.04	1.54	1.17	1.25	0.86	0.84	0.77
Plate counting ^c	1.3×10^3	1.4×10^3	1.5×10^3	1.0×10^7	2.5×10^6	3.1×10^6	3.7×10^4	4.2×10^4	7.5×10^4
qPCR ^d	3.6×10^5	5.0×10^5	2.2×10^5	4.9×10^6	3.0×10^6	1.9×10^6	8.3×10^5	4.0×10^6	5.8×10^6
QX200 ^e	1.3×10^5	2.2×10^5	1.6×10^5	1.7×10^7	5.5×10^6	8.2×10^6	1.1×10^5	1.0×10^6	6.7×10^5
QS3D ^e	5.0×10^4	2.2×10^5	1.3×10^5	1.9×10^7	6.6×10^6	5.8×10^6	6.5×10^5	6.5×10^5	7.1×10^5

The results are referred to the initial unknown suspensions before dilution.

^aNumber of MAP cells/ μ L evaluated by Burker chamber, counting 20 squares and calculating the final result with the web tool available at the web site of "The Ebert Group" (<http://evolution.unibas.ch/ebert/lab/counting.htm>).

^bAbsorbance recorded at 600 nm.

^cNumber of bacteria in the unknown water suspensions evaluated by cultural plating in appropriate medium, for more details refer to material and method section. Results are expressed as CFU/ μ L.

^dFor MAP, it was evaluated by multiplying per ten the number of bacteria recovered at the dilution -1 . Results are expressed as number of cells/ μ L.

^eEvaluated by multiplying for the Log_{10} factor from the first dilution in which it was possible to count the number of bacteria. Results are expressed as number of cells/ μ L.

TABLE 6 | Level of uncertainty relative to *L. monocytogenes* for all the methods.

	Uncertainty
Plate counting	0.208
qPCR	0.062
QX200	0.113
QS3D	0.167

Data were Log_{10} transformed before uncertainty's evaluation according to the Material and Method section.

avoid any bias in the determination of the LOD during the PCR assay validation, this difference should be taken into account (Versage et al., 2003). In fact, to bypass this problem, the most recently developed methods have used genomic pure DNA or plasmid standards instead of pure cultures of *Francisella* (Euler et al., 2012; Seiner et al., 2013).

On the contrary, no differences were found for *L. monocytogenes* (24h of growth in blood agar), between plate counting and PCRs. This suggests the possibility to quantify *L. monocytogenes* with molecular assays, which seems to be a reliable alternative to the cultural method. In this context, for *L. monocytogenes*, a quantitative maximum limit of contamination, is stated by the Reg EC 2073/2005, which in turn defines the microbiological criteria for foodstuffs (Anonymous, 2005). The level defined for *L. monocytogenes* is " ≤ 100 CFU/g for Ready To Eat (RTE) foodstuffs." Notably, the analytical time for traditional microbiological methods varies from 2 to 3 days, but, it can even take up to a week before a final result is achieved for positive samples. This could be a serious problem for the commercialization of RTE products, because often they have a short shelf-life.

In addition, since *L. monocytogenes* is the only pathogen in which a quantitative maximum limit has been defined (100 CFU/g), it is important to express the uncertainty associated

with the use of PCR approaches and compare it to that for cultural assay (Anonymous, 2009). Our results suggest the level of uncertainty of both qPCR and dPCRs was similar or lower to that calculated for the cultural assay (Table 6). This result clearly demonstrated how PCR approaches are suitable for the quantification and can represent a valid alternative for the enumeration of *L. monocytogenes*.

In conclusion, the quantifications of MAP, *L. monocytogenes* and *F. tularensis* by the two dPCR platforms were highly comparable to each other. However, the comparison between qPCR and dPCR suggested some differences are present. Probably, it is not always possible to pass between qPCR and dPCR without any optimization of the concentration of primers and probes. One of the critical points for the enumeration by qPCR can be the difficulty in the quantification of the standards needed for the building of the calibration curves. This issue represents a challenging factor for the standardization of a quantifying method and also implies a higher reagents cost. Notably, the request of requirements for international standards for molecular biology assays is increasing and, since the production of useful molecular biology reference materials poses some technical challenges, one European project, the "Metrology for Monitoring Infectious Diseases, Antimicrobial Resistance and Harmful Micro-organisms," also addressed this purpose (Pavšič et al., 2015). If more reference material becomes available, we believe PCRs approaches can become the new gold standard methods for the quantification of bacterial pathogens.

AUTHOR CONTRIBUTIONS

MR, MBB, NV, and BB conceived, designed and wrote the paper. CB helped to write the paper and performed the experiments with QX200 dPCR. SR performed the quantification by qPCR and other methods for MAP. MT performed the experiment about *L. monocytogenes* and all experiment with Quant Studio 3D

dPCR. NV and MAB performed the quantification by qPCR and other methods for *F. tularensis*.

ACKNOWLEDGMENTS

This work was supported by Public Health Service grant E88F15000140001 (IZSLER PRC2014-013) from the Italian ministry of Health. We thank Mr. Walter Zeni from the University of Milan for his help in the building of the graphs. We thank Dr. Plain from the University of Sidney for

providing MAP DNA. We thank Dr. Enrico Pavoni for his help during the revision of the manuscript. Finally, we thank Mr. Bryan Manchi for his valuable revision of the English text.

SUPPLEMENTARY MATERIAL

The Supplementary Material for this article can be found online at: <http://journal.frontiersin.org/article/10.3389/fmicb.2017.01174/full#supplementary-material>

REFERENCES

- Anonymous (1998). *ISO 11290-2: Microbiology of Food and Animal Feeding Stuffs - Horizontal Method for the Detection and Enumeration of Listeria monocytogenes - Part 2: Enumeration Method*. Geneva.
- Anonymous (2005). *COMMISSION REGULATION (EC) No 2073/2005 of 15 November 2005 on Microbiological Criteria for Foodstuffs*. Rome.
- Anonymous (2009). *ISO/TS 19036:2006: Microbiology of Food and Animal Feeding Stuffs - Guidelines for the Estimation of Measurement Uncertainty for Quantitative Determinations*. Geneva: AMEDMENT 1.
- Anonymous (2012). *ISO/TS 12869: Water quality - Detection and Quantification of Legionella spp. and/or Legionella pneumophila by Concentration and Genic Amplification by Quantitative Polymerase Chain reaction (qPCR)*. Geneva.
- Anonymous (2014). *OIE Validation Guidelines (2014). VALIDATION GUIDELINE 3.6.5. STATISTICAL APPROACHES TO VALIDATION*. Paris: World Organisation for Animal Health, 1–12.
- Bland, J. M., and Altman, D. G. (1986). Statistical methods for assessing agreement between two methods of clinical measurement. *Lancet* 1, 307–310. doi: 10.1016/S0140-6736(86)90837-8
- Boizeau, L., Laperche, S., Desire, N., Jourdain, C., Thibault, V., and Servant-Delmas, A. (2014). Could droplet digital PCR be used instead of real-time PCR for quantitative detection of the hepatitis B virus genome in plasma? *J. Clin. Microbiol.* 52, 3497–3498. doi: 10.1128/jcm.01306-14
- Boulais, C., Wacker, R., Augustin, J. C., Cheikh, M. H., and Peladan, F. (2011). Modeling the occurrence of *Mycobacterium avium* subsp. *paratuberculosis* in bulk raw milk and the impact of management options for exposure mitigation. *J. Food Prot.* 74, 1126–1136. doi: 10.4315/0362-028X.JFP-11-005
- Burns, M., and Valdivia, H. (2008). Modelling the limit of detection in real-time quantitative PCR. *Eur. Food Res. Technol.* 226:12. doi: 10.1007/s00217-007-0683-z
- Bustin, S. A., Benes, V., Garson, J. A., Hellems, J., Huggett, J., Kubista, M., et al. (2009). The MIQE guidelines: minimum information for publication of quantitative real-time PCR experiments. *Clin. Chem.* 55, 611–622. doi: 10.1373/clinchem.2008.112797
- Carvalho, C. L., Lopes de Carvalho, I., Ze-Ze, L., Nuncio, M. S., and Duarte, E. L. (2014). Tularaemia: a challenging zoonosis. *Comp. Immunol. Microbiol. Infect. Dis.* 37, 85–96. doi: 10.1016/j.cimid.2014.01.002
- Chiodini, R. J., Chamberlin, W. M., Sarosiek, J., and McCallum, R. W. (2012). Crohn's disease and the mycobacterioses: a quarter century later. Causation or simple association? *Crit. Rev. Microbiol.* 38, 52–93. doi: 10.3109/1040841X.2011.638273
- Devonshire, A. S., Honeyborne, I., Gutteridge, A., Whale, A. S., Nixon, G., Wilson, P., et al. (2015). Highly reproducible absolute quantification of *Mycobacterium tuberculosis* complex by digital PCR. *Anal. Chem.* 87, 3706–3713. doi: 10.1021/ac5041617
- Devonshire, A. S., O'Sullivan, D. M., Honeyborne, I., Jones, G., Karczmarczyk, M., Pavšič, J., et al. (2016). The use of digital PCR to improve the application of quantitative molecular diagnostic methods for tuberculosis. *BMC Infect. Dis.* 16:366. doi: 10.1186/s12879-016-1696-7
- Euler, M., Wang, Y., Otto, P., Tomaso, H., Escudero, R., Anda, P., et al. (2012). Recombinase polymerase amplification assay for rapid detection of *Francisella tularensis*. *J. Clin. Microbiol.* 50, 2234–2238. doi: 10.1128/JCM.06504-11
- Gosselin-Theberge, M., Taboada, E., and Guy, R. A. (2016). Evaluation of real-time PCR assays and standard curve optimisation for enhanced accuracy in quantification of *Campylobacter* environmental water isolates. *J. Microbiol. Methods* 129, 70–77. doi: 10.1016/j.mimet.2016.07.025
- Halder, A., Black, D. G., Davidson, P. M., and Datta, A. (2010). Development of associations and kinetic models for microbiological data to be used in comprehensive food safety prediction software. *J. Food Sci.* 75, R107–R120. doi: 10.1111/j.1750-3841.2010.01687.x
- Hayden, R. T., Gu, Z., Ingersoll, J., Abdul-Ali, D., Shi, L., Pounds, S., et al. (2013). Comparison of droplet digital PCR to real-time PCR for quantitative detection of cytomegalovirus. *J. Clin. Microbiol.* 51, 540–546. doi: 10.1128/JCM.02620-12
- Herthnek, D., Nielsen, S. S., Lindberg, A., and Bölske, G. (2008). A robust method for bacterial lysis and DNA purification to be used with real-time PCR for detection of *Mycobacterium avium* subsp. *paratuberculosis* in milk. *J. Microbiol. Methods* 75, 335–340. doi: 10.1016/j.mimet.2008.07.009
- Hoshino, T., and Inagaki, F. (2012). Molecular quantification of environmental DNA using microfluidics and digital PCR. *Syst. Appl. Microbiol.* 35, 390–395. doi: 10.1016/j.syapm.2012.06.006
- Hudecova, I. (2015). Digital PCR analysis of circulating nucleic acids. *Clin. Biochem.* 48, 948–956. doi: 10.1016/j.clinbiochem.2015.03.015
- Huggett, J. F., Foy, C. A., Benes, V., Emslie, K., Garson, J. A., Haynes, R., et al. (2013). The digital MIQE guidelines: minimum information for publication of quantitative digital PCR experiments. *Clin. Chem.* 59, 892–902. doi: 10.1373/clinchem.2013.206375
- Kralik, P., Beran, V., and Pavlik, I. (2012). Enumeration of *Mycobacterium avium* subsp. *paratuberculosis* by quantitative real-time PCR, culture on solid media and optical densitometry. *BMC Res. Notes* 5:114. doi: 10.1186/1756-0500-5-114
- Law, J. W., Ab Mutalib, N. S., Chan, K. G., and Lee, L. H. (2014). Rapid methods for the detection of foodborne bacterial pathogens: principles, applications, advantages and limitations. *Front. Microbiol.* 5:770. doi: 10.3389/fmicb.2014.00770
- Logar, K., Kopinč, R., Bandelj, P., Starič, J., Lapanje, A., and Ocepek, M. (2012). Evaluation of combined high-efficiency DNA extraction and real-time PCR for detection of *Mycobacterium avium* subsp. *paratuberculosis* in subclinically infected dairy cattle: comparison with faecal culture, milk real-time PCR and milk ELISA. *BMC Vet. Res.* 8:49. doi: 10.1186/1746-6148-8-49
- Nauta, M. J., and van der Giessen, J. W. (1998). Human exposure to *Mycobacterium paratuberculosis* via pasteurised milk: a modelling approach. *Vet. Rec.* 143, 293–296. doi: 10.1136/vr.143.11.293
- Papic, B., Pate, M., Henigman, U., Zajc, U., Gruntar, I., Biasizzo, M., et al. (2017). New approaches on quantification of campylobacter jejuni in poultry samples: the use of digital PCR and real-time PCR against the ISO standard plate count method. *Front. Microbiol.* 8:331. doi: 10.3389/fmicb.2017.00331
- Pavšič, J., Devonshire, A. S., Parkes, H., Schimmel, H., Foy, C. A., Karczmarczyk, M., et al. (2015). Standardization of nucleic acid tests for clinical measurements of bacteria and viruses. *J. Clin. Microbiol.* 53, 2008–2014. doi: 10.1128/JCM.02136-14
- Pavšič, J., Zel, J., and Milavec, M. (2016). Assessment of the real-time PCR and different digital PCR platforms for DNA quantification. *Anal. Bioanal. Chem.* 408, 107–121. doi: 10.1007/s00216-015-9107-2
- Plain, K. M., Marsh, I. B., Waldron, A. M., Galea, F., Whittington, A. M., Saunders, V. F., et al. (2014). High-throughput direct fecal PCR assay for detection

- of *Mycobacterium avium* subsp. paratuberculosis in sheep and cattle. *J. Clin. Microbiol.* 52, 745–757. doi: 10.1128/JCM.03233-13
- Ricchi, M., De Cicco, C., Kralik, P., Babak, V., Boniotti, M. B., Savi, R., et al. (2014). Evaluation of viable *Mycobacterium avium* subsp. paratuberculosis in milk using peptide-mediated separation and Propidium Monoazide qPCR. *FEMS Microbiol. Lett.* 356, 127–133. doi: 10.1111/1574-6968.12480
- Ricchi, M., Savi, R., Bolzoni, L., Pongolini, S., Grant, I. R., De Cicco, C., et al. (2016). Estimation of *Mycobacterium avium* subsp. paratuberculosis load in raw bulk tank milk in Emilia-Romagna Region (Italy) by qPCR. *Microbiologyopen*. 5, 551–559. doi: 10.1002/mbo3.350
- Rothrock, M., Hiatt, K. L., Kiepper, B. H., Ingram, K., and Hinton, A. (2013). Quantification of zoonotic bacterial pathogens within commercial poultry processing water samples using droplet digital PCR. *Adv. Microbiol.* 3:403. doi: 10.4236/aim.2013.35055
- Seiner, D. R., Colburn, H. A., Baird, C., Bartholomew, R. A., Straub, T., Victry, K., et al. (2013). Evaluation of the FilmArray[®] system for detection of *Bacillus anthracis*, *Francisella tularensis* and *Yersinia pestis*. *J. Appl. Microbiol.* 114, 992–1000. doi: 10.1111/jam.12107
- Sloots, T. P., Nissen, M. D., Ginn, A. N., and Iredell, J. R. (2015). Rapid identification of pathogens using molecular techniques. *Pathology* 47, 191–198. doi: 10.1097/PAT.0000000000000241
- Tasara, T., and Stephan, R. (2005). Development of an F57 sequence-based real-time PCR assay for detection of *Mycobacterium avium* subsp. paratuberculosis in milk. *Appl. Environ. Microbiol.* 71, 5957–5968. doi: 10.1128/AEM.71.10.5957-5968.2005
- Traunsek, U., Toplak, N., Jersek, B., Lapanje, A., Majstorovic, T., and Kovac, M. (2011). Novel cost-efficient real-time PCR assays for detection and quantitation of *Listeria monocytogenes*. *J. Microbiol. Methods* 85, 40–46. doi: 10.1016/j.mimet.2011.01.018
- Verhaegen, B., De Reu, K., De Zutter, L., Verstraete, K., Heyndrickx, M., and Van Coillie, E. (2016). Comparison of droplet digital PCR and qPCR for the quantification of shiga toxin-producing *Escherichia coli* in bovine feces. *Toxins (Basel)* 8:E157. doi: 10.3390/toxins8050157
- Versage, J. L., Severin, D. D., Chu, M. C., and Petersen, J. M. (2003). Development of a multitarget real-time TaqMan PCR assay for enhanced detection of *Francisella tularensis* in complex specimens. *J. Clin. Microbiol.* 41, 5492–5499. doi: 10.1128/JCM.41.12.5492-5499.2003
- Wang, D., Yamahara, K. M., Cao, Y., and Boehm, A. B. (2016). Absolute quantification of enterococcal 23S rRNA gene using digital PCR. *Environ. Sci. Technol.* 50, 3399–3408. doi: 10.1021/acs.est.5b05747
- Witte, A. K., Fister, S., Mester, P., Schoder, D., and Rossmann, P. (2016). Evaluation of the performance of quantitative detection of the *Listeria monocytogenes* prfA locus with droplet digital PCR. *Anal. Bioanal. Chem.* 408, 7583–7593. doi: 10.1007/s00216-016-9861-9
- Wood, R. M., Egan, J. R., and Hall, I. M. (2014). A dose and time response Markov model for the in-host dynamics of infection with intracellular bacteria following inhalation: with application to *Francisella tularensis*. *J. R. Soc. Interface* 11:20140119. doi: 10.1098/rsif.2014.0119

Conflict of Interest Statement: The authors declare that the research was conducted in the absence of any commercial or financial relationships that could be construed as a potential conflict of interest.

Copyright © 2017 Ricchi, Bertasio, Boniotti, Vicari, Russo, Tilola, Bellotti and Bertasi. This is an open-access article distributed under the terms of the Creative Commons Attribution License (CC BY). The use, distribution or reproduction in other forums is permitted, provided the original author(s) or licensor are credited and that the original publication in this journal is cited, in accordance with accepted academic practice. No use, distribution or reproduction is permitted which does not comply with these terms.